

Anna Bogdan,  
Iwona Sudol-Szopińska,  
\*Tomasz Szopiński

Department of Ergonomics, Central Institute for  
Labour Protection - National Research Institute,  
00-701 Warsaw, ul. Czerniakowska 16, Poland

\*Department of Urology,  
Central Railway Hospital,  
ul. Bursztynowa 2, 04-749 Warsaw, Poland  
E-mail: anbog@ciop.pl

# Assessment of Textiles for Use in Operating Theatres with Respect to the Thermal Comfort of Surgeons

## Abstract

*Materials used to manufacture surgical clothing ensembles are characterised by high barrier-properties protecting surgeons and patients against germs. However, medical clothing made of those materials should not induce thermal stress. Such an uncomfortable sensation experienced by surgeons can decrease their psychomotor skills and, at the same time, adversely influence the way an operation procedure is carried out. The objective of this paper is to present a problem which affects the majority of surgeons: the too high thermal insulation of medical clothing ensembles, which results in thermal stress experienced by this professional group.*

**Key words:** medical protective clothing, thermal insulation, thermal manikin, medical standards.

## Introduction

Medical clothing for personnel working in an operating theatre must be made of materials resistant to the permeation of blood and other body liquids, as well as to germs transferred by them. Moreover it has to meet the requirements of the PPE (Personal Protective Equipment) directive [1] and harmonised Standard EN 13795 1-3 [2 - 4]. The aforementioned standard, in annex A [2], mentions the need of assessing materials and medical clothing also in terms of ensuring thermal comfort, i.e. "surgical clothing should be designed in a manner which will minimise physiological stress related to work in this type of clothing". Furthermore, the standard points to the need for carrying out an assessment of thermal resistance, air permeability, water steam-resistance and flexibility. However, no concrete values of the parameters mentioned are given.

One of the establishments which deals with the testing of medical clothing is the Hohenstein Institute, Germany. Scientists from this Institute introduced a certificate called the Hohenstein Quality Label 'Breathability', which is granted to medical clothing whose steam water resistance, measured on a skin model compliant with Standard EN 31092 [5], is below 17 m<sup>2</sup>Pa/W. This value was set on the basis of experiments conducted by Bartels [6], which established a correlation between the steam water resistance of barrier material and the maximum temperature of the environment at which the user continues to experience thermal comfort. Apart from steam water permeation, the thermal comfort of the user of medical clothing depends, above all, on the thermal insulation and its adjustment to

environmental conditions existing in an operating theatre during a surgical operation. Thermal insulation tests performed at the Central Institute of Labour Protection – National Research Institute on surgical clothing ensembles in the past years, selected in accordance with WHO recommendations and the requirements of EN ISO 9001 [7], showed that their thermal insulation lies within the limits:  $0.54 \pm 0.01$  clo -  $0.95 \pm 0.01$  clo [8]. At the same time, it was determined that surgeons will experience thermal comfort when the temperature in an operating theatre amounts to 20 - 24 °C and their clothing is composed of shoes, cotton socks and a surgical ensemble made of nonwoven fabric, similar to cotton, containing viscose fibres of good air and water steam permeability. Likewise, thermal comfort can also be achieved in the temperature range of 16 - 20 °C, when the surgical outfit includes the above-mentioned garment in combination with a thermoplastic 2-layered hygienic surgical gown, a made of nonwoven fabric and polypropylene foil, which is liquid-proof.

Due to the fact that medical clothing made of cotton material is being gradually taken out of use and in light of the need signalled in the standard [2] to search for assessment methods which take into account the thermal comfort of medical clothing, the authors of this paper decided to conduct their own tests. Contrary to the testing of materials carried out by the Hohenstein Institute, the authors performed tests on full ensembles of medical clothing. Objective research results were supplemented by an analysis of the physiological parameters of surgeons as well as their subjective assessment.

## Objective of the study

the main goal of this study was to assess the thermal insulation of modern materials used in manufacturing medical clothing in the context of thermal comfort experienced by surgeons wearing a full clothing ensemble. Furthermore, in order to confirm our considerations, it was decided to conduct a case study – a physiological examination of surgeons using selected clothing ensembles in real-life surgery – a urological procedure. Due to the difficulty of carrying out a medical examination during real-life surgery, the number of subjects was limited to 2 surgeons.

## Material and methods

in order to examine the thermal insulation of surgical gowns against the requirements of thermal comfort, the thermal parameters were tested in operating theatres. Thermal insulation was measured for selected ensembles of medical clothing, and next the results were compared with guidelines on the thermal insulation required to achieve thermal comfort when performing work in an operating theatre.

Additionally the physiological parameters of surgeons were assessed during the performance of surgery in a given clothing ensemble.

## Microclimate measurements

The microclimate in an operating theatre was tested with the use of MM-01 microclimate meters, located near a surgeon (measurement points 1 and 2). The tests were performed during the real time of a surgical procedure. Measurements were



**Figure 1.** Thermal manikin wearing ensembles of surgical gowns (A – surgical underwear and ensemble A, B – surgical underwear and ensemble B; C - surgical underwear and ensemble C; D - surgical underwear and ensemble D).

made in 2 operating theatres (A and B) of the Specialised Hospital in Warsaw, which has environmental conditions compliant with Polish regulations [9].

Measurements of the microclimate parameters were determined by the PVM index (which represents the overall thermal sensation). PVM is described with the following values: -3 cold, -2 cool, -1 slightly cool, 0 – neutral, +1 slightly warm, +2 warm, +3 hot. Thermal comfort ranges within the limits  $-0.5 < PMV < +0.5$  [11]

### Testing ensembles of surgical clothing

Four clothing ensembles and one underwear ensemble used with surgical gowns were selected for the purpose of this study (Figure 1). They represented typical disposable medical clothing manufactured according to the requirements of EN ISO 9001 [7] and EN 13795 [2 - 4]:

- **Ensemble A** - barrier surgical gown for multiple use, worn during standard risk operations, made of polyester cloth with the addition of carbon fibre. The gown's critical area (front and sleeves) is made of liquid proof fabric of higher resistance (weight 300 g)
- **Ensemble B** - barrier surgical gown for multiple use, worn during high

risk operations, made of polyester cloth with the addition of carbon fibre on the back. The gown's critical area (front and sleeves) is made of laminate with a PTFE (polytetrafluorethylene) membrane

- **Ensemble C** – cotton surgical gown for single use (in theory, whose use is discontinued, yet it is still worn in operating theatres)
- **Ensemble D** - lead surgical apron, Pb 0.5 mm, used to make x-ray pictures (mass 3.349 kg).

The surgical underwear applied in all the test variants was identical - made of polyester cloth with coal fibre, ensuring humidity absorption from the skin's surface.

### Thermal insulation measurements

All the experiments were performed on a thermal manikin and took place in a walk-in climatic chamber. The thermal insulation of the ensembles was determined on a thermal stand, a stationary manikin type TM 3.2/R110, named 'Diana', [8]. Measurements were taken in accordance with Standard EN ISO 15831 [10]. Each measurement was repeated three times with the assumption that the climatic chamber had the following environmental parameters: air temperature ( $t_a$ )  $20 \pm 0.1$  °C, air velocity ( $v_a$ )  $0.4 \pm 0.05$  m/s, and relative humidity (RH)  $45 \pm 1\%$ . All the measurements were taken at 1-second intervals, and subsequently a 1-minute average value was calculated and recorded. The results were constantly displayed to help evaluate the steady state.

**Table 1.** Physical characteristics of the subjects. (\* $A_{Du}$  Body area by Hardy and DuBois [13]).

Parameter	Subject	
	1	2
Weight, kg	81	103
Height, m	1.78	1.80
$A_{Du}^*$ , m <sup>2</sup>	1.99	2.22
Age, years	38	45

### Case study with the participation of surgeons

In the case study experiments in an operation theatre, two surgeons were subjected to experiment. Both men were in a good physical state, the physical characteristics of which are presented in Table 1.

Measurements of the surgeons' skin temperature were taken at 4 measurement points (a sensor closely fastened to the skin's surface) as well as measurements of the temperature and humidity between the skin of the subject and his clothing (sensors were placed on the stand 2 mm away from the skin's surface) (Figure 2). The experiments were performed with the use of a HygroLab2 (manufactured by Rotronic AG) and cardio monitor FX 2000 (manufactured by Emtel). The testing procedure was approved by the Committee for Research Ethics.

Each surgeon took part in the experiment four times, i.e. in each of the four clothing ensembles:

- surgical underwear, cotton gown (C) and lead gown (D)
- surgical underwear and cotton gown (C)
- surgical underwear and polyester gown (A)
- surgical underwear and polyester gown (B).


### Results

#### Results of experiments on the thermal environment in an operating theatre

On the basis of the measurements made in two operating theatres, the PMV index was specified at two measurement locations corresponding to those where the surgeons stood at the operating table (1 and 2) in two operating theatres (A and B) of the hospital (Table 2). The PMV was calculated on the basis of the programme available in the ISO 7730 standard [14]. The PMV index values calculated for surgeons wearing each of the test surgical clothing ensembles showed that their

**Table 2.** Air parameters in operating theatres ( $t_a$  – ambient temperature, RH – relative humidity,  $v_a$  – air velocity).

Operating theatre	Measurement point	$t_a$ , °C	RH, %	$v_a$ , m/s
A	1	22.9	54.6	0.1
	2	24.6	66.0	0.0
B	1	22.9	54.6	0.0
	2	24.6	66	0.0

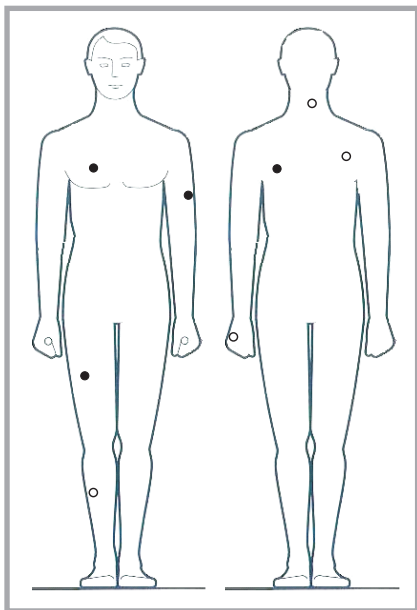

**Figure 2.** Distribution of sensors for the measurement of skin temperature ( $t_{skin}$ ) as well as the temperature and humidity in the area between the clothing and the body ( $t_s$ , and  $RH_s$ ).

thermal sensation is defined at a PMV level ranging between +0.75 and +1.25. From this, it follows that surgeons assess the thermal environment from “slightly warm” to “warm”. As for the patient on which surgery was performed, the PMV index amounted to -2 (‘cool’ thermal sensation). The results obtained showed that limiting control to thermal environment parameters only does not ensure the patient nor medical personnel thermal comfort at the same time. For this reason the only possibility of providing a surgeon with thermal comfort is to select the properties of the clothing he/she uses in an appropriate manner.

**Figure 3** presents a graph with values of the PMV index determined on the basis of the thermal insulation of the clothing ensemble used. These values were established considering the arithmetic mean of the air parameters measured for the operating theatres. On the basis of the graph, it can be observed that approaching conditions considered comfortable is only possible in the case of surgical clothing within the value range of 0.028 m<sup>2</sup>K/W and 0.124m<sup>2</sup>K/W

### Results of tests on the thermal insulation of surgical clothing

The results of tests examining the thermal insulation of the given clothing ensembles (surgical underwear and gown) and surgical underwear are presented in

**Table 3.** It can be concluded that the insulation value of particular ensembles of surgical underwear and surgical gowns are comparable, with the highest insulation value being noted in the case of the cotton gown ensemble. Furthermore It was noted that the thermal insulation of surgical underwear and lead gowns is lower than ensembles with other surgical gowns, which would indicate that a lead gown constitutes some sort of load for the surgeon’s body, which is only due to its weight (3.3 kg) and not because of its high insulation. The results have also demonstrated that the highest insulation is possessed by surgical underwear used under all types of surgical gowns.

Comparison of the results obtained with **Figure 3** revealed that clothing ensembles currently used are characterised by too high insulation values in relation to the value required for maintaining thermal comfort. The highest thermal value is possessed by surgical clothing worn under a surgical gown; therefore, for thermal comfort to be achieved, it is necessary to decrease the insulation value of surgical underwear to ca. 0.08 m<sup>2</sup>K/W

### Case study experiments

**Figures 4 - 6** show differences in the physiological parameters of both surgeons (mean skin temperature, mean temperature and humidity in the space between the skin and the inner layer of the clothing, as well as the perspiration rate) when performing surgical treatment in four clothing ensembles. The highest increase in the mean skin temperature during an operation was observed with surgeon 1 wearing surgical underwear and a cotton gown (C), whereas with surgeon 2 this occurred during an operation conducted in a polyester gown. The highest increase in the mean temperature in the area between the skin and clothing was observed when surgeon 1 performed an operation wearing surgical underwear

and a cotton gown (C), whereas with surgeon 2 this occurred during surgery in surgical underwear and a polyester gown (B). The highest increase in mean humidity in the area between the skin and clothing was observed when surgeon 1 performed surgical treatment using surgical underwear and a cotton gown (C), whereas with a surgeon 2 this occurred during an operation in surgical underwear and a cotton gown together with a lead apron (C and E).


Following these findings, it can be concluded that the objective maximum thermal discomfort experienced by surgeon 1 occurred when performing surgical treatment in a cotton gown (C) and was slightly smaller in a medical clothing ensemble with a polyester gown equipped with a PTFE membrane (B). As regards thermal comfort, it was maintained during the performance of surgery in a polyester gown (A). With regard to surgeon 2, the highest thermal discomfort level appeared during an operation performed in a polyester gown with a PTFE membrane (B); it was smaller in a cotton gown (C). Under none of the experiment variants was thermal comfort achieved with surgeon 2. In the case of both surgeons, a considerable increase in humidity in the area between the skin and clothing was noted, attributed to insufficient sweat transfer from the surface of the surgeon’s body.

The results of the case study revealed no major difference in the clothing ensembles examined. However, they have confirmed the need for further study into the thermal comfort of surgeons performing surgery in protective clothing. Furthermore, the results have shown weak points in the clothing structure e.g. a considerable increase in the mean skin temperature by almost 2 °C and in the humidity between the skin and clothing by 40%. This information should be used by clothing


**Table 3.** Thermal insulation for given ensembles of surgical clothing (thermal insulation nomenclature of EN ISO 15831).

Type of clothing	Thermal insulation, m <sup>2</sup> K/W	
	parallel	serial
Surgical underwear + polyester gown (ensemble A)	0.151	0.202
Surgical underwear + polyester gown (ensemble B)	0.160	0.218
Surgical underwear + cotton gown (ensemble C)	0.166	0.231
Surgical underwear + lead gown (ensemble D)	0.149	0.193
Surgical underwear	0.123	0.154




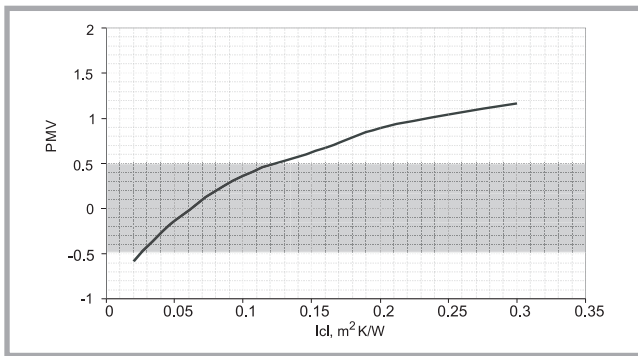


**Figure 3.** Changes in the PMV index with respect to the thermal insulation values of clothing ensembles (grey field marks the thermal comfort zone).

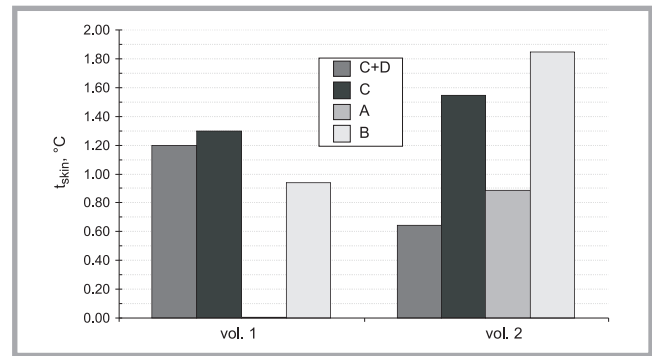

**Figure 4.** Increase in the mean skin temperature of a surgeon ( $t_{skin}$ ) during a surgical operation for each variant of the experiment.

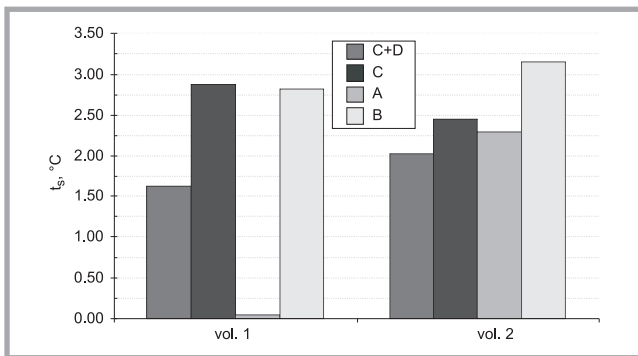

**Figure 5.** Increase in the mean temperature in the area between the skin and inner layer of a surgeon's clothing ( $t_s$ ) during a surgical operation for each variant of the experiment.

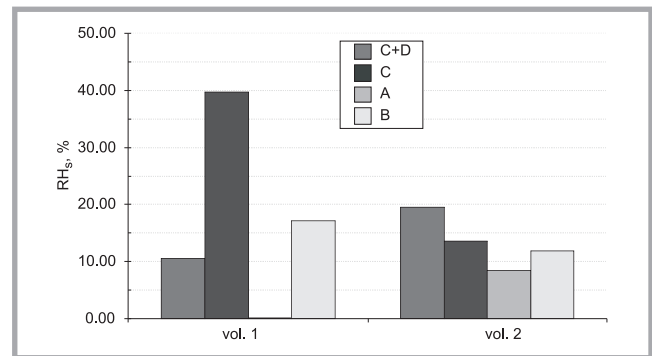

**Figure 6.** Increase in mean humidity in the area between the skin and inner layer of a surgeon's clothing ( $RH_s$ ) during a surgical operation for each variant of the experiment.

designers as a guideline when creating new types of protective garment.

## Conclusions

It is crucial that surgical clothing protect the surgeon and patient from infecting each other. It follows that the key parameters which need to be observed, in compliance with Standard EN 13795 [2 - 4], include the following features: germ-resistance, pollen-resistance, cleanliness, liquid-resistance, and material resistance to bagging and stretching. It should also be borne in mind that surgical work is performed in a high air temperature environment, requiring psycho-physical fitness.

On the basis of the experiments conducted, the following conclusions were drawn:

1. The clothing ensembles tested are characterised by too high thermal insulation in relation to the value required for maintaining thermal comfort conditions. The highest thermal insulation is characterised by surgical underwear made of polyester cloth with carbon fibre, which, in theory,

was supposed to be characterised by high humidity absorption.

2. Air parameters are not appropriate to ensure the surgeon and patient thermal comfort at the same time. Comfort conditions for the surgeon can be achieved only when surgical clothing insulation has a value within a range of 0.028 m<sup>2</sup>K/W (0.18 clo) and 0.124 m<sup>2</sup>K/W (0.8 clo).
3. On the basis of the results of the physiological parameters of surgeons in this case study, it was determined that in all the types of clothing ensembles tested, the skin temperature as well as the temperature and humidity in the area between the skin and clothing would increase.
4. The most negative assessment of the thermal environment was noted during experiments in a cotton gown and lead gown protecting against X-rays (used more and more often due to the development of minimally-invasive surgical techniques).

The results obtained leave no doubt that work which is performed in medical clothing made of latest technology materials entails considerable thermal dis-

comfort for a surgeon. The unduly high insulation of medical clothing ensembles and too low absorption of surgical inner clothing result in an increase in skin temperature, which also induces a high accumulation of humidity in the area between the skin and clothing, which can result in a worsening of the psycho-physical condition of surgeons.

Given that the correct course of a surgical procedure depends, to a large extent, on the surgeon's mental condition, inter alia, on their ability to maintain constant vigilance and concentration [12], the elimination of cotton gowns was an important step towards improving safety in an operating theatre. However, as our experiments have shown, medical clothing ensembles made of modern materials can still bring about the risk of thermal stress.

## Acknowledgment

The publication was prepared within the framework of the project „Assessment of the physiological properties of surgical clothing in order to ensure thermal comfort“ carried out at the 1st stage of the National Programme: „Improvement of safety and working conditions“. Financial assistance for the years 2008-2010 has been provided by the Ministry of Labour

and Social Policy within the scope of tasks related to services to the State. Main coordinator - Central Institute for Labour Protection - National Research Institute.

## References

1. Council Directive 89/686/EEC of 21 December 1989 on the approximation of the laws of the Member States relating to personal protective equipment.
2. EN 13795-1, Surgical drapes, gowns and clean air suits, used as medical devices, for patients, clinical staff and equipment. General requirements for manufacturers, processors and products.
3. EN 13795-2, Surgical drapes, gowns and clean air suits, used as medical devices for patients, clinical staff and equipment. Test methods.
4. EN 13795-3, Surgical drapes, gowns and clean air suits, used as medical devices for patients, clinical staff and equipment. Performance requirements and performance levels.
5. EN 31092, Textiles. Determination of physiological properties. Measurement of thermal and water-vapour resistance under steady-state conditions (sweating guarded-hotplate test).
6. Bartels V. T., Umbach K. H.; Psychological function and wear comfort of protective clothing with the examples of OR-gowns and fire fighters garments, Proceedings 4. Int. Conference on Safety and Protective Fabrics, Pittsburgh, USA, 2004.
7. EN ISO 9001, Quality management systems. Requirements.
8. Konarska M., Soltynski K., Sudol-Szopinska I., Chojnacka A.; Comparative evaluation of clothing thermal insulation measured on a thermal manikin and on volunteers, *Fibres & Textiles in Eastern Europe* April / June 2007, Vol. 15, No. 2 (61), pp. 79-85.
9. Ordinance of Ministry of Health of the Republic of Poland (Journal of Laws from 2006 No 213, entry 1568).
10. EN ISO 15831, Clothing - Physiological effects - Measurement of thermal insulation by means of a thermal manikin.
11. Fanger P.O., (1970) *Thermal comfort*, McGraw-Hill, New York, 1970.
12. Pilcher J. J., Nadler, E., Busch, C.; Effects of hot and cold temperature exposure on performance: a meta-analytic review. *Ergonomics*, Vol. 45, No. 10, (2002), pp. 682-698.
13. DuBois D, DuBois E. F.; A formula to estimate surface area in height and weight are known, *Archives of Internal Medicine*, Vol. 17, (1916) p. 863.
14. ISO 7730:2005, Ergonomics of the thermal environment. Analytical determination and interpretation of thermal comfort using calculation of the PMV and PPD indices and local thermal comfort criteria.

Received 27.01.2010 Reviewed 12.03.2010



# INSTITUTE OF BIOPOLYMERS AND CHEMICAL FIBRES

## LABORATORY OF ENVIRONMENTAL PROTECTION

The Laboratory works and specialises in three fundamental fields:

### R&D activities:

- research works on new technology and techniques, particularly environmental protection;
- evaluation and improvement of technology used in domestic mills;
- development of new research and analytical methods;

■ **research services** (measurements and analytical tests) in the field of environmental protection, especially monitoring the emission of pollutants;

■ **seminar and training activity** concerning methods of instrumental analysis, especially the analysis of water and wastewater, chemicals used in paper production, and environmental protection in the paper-making industry.

**Since 2004 Laboratory has had the accreditation of the Polish Centre for Accreditation No. AB 551, confirming that the Laboratory meets the requirements of Standard PN-EN ISO/IEC 17025:2005.**



AB 388

### Investigations in the field of environmental protection technology:

- Research and development of waste water treatment technology, the treatment technology and abatement of gaseous emissions, and the utilisation and reuse of solid waste,
- Monitoring the technological progress of environmentally friendly technology in paper-making and the best available techniques (BAT),
- Working out and adapting analytical methods for testing the content of pollutants and trace concentrations of toxic compounds in waste water, gaseous emissions, solid waste and products of the paper-making industry,
- Monitoring ecological legislation at a domestic and world level, particularly in the European Union.

### A list of the analyses most frequently carried out:

- Global water & waste water pollution factors: COD, BOD, TOC, suspended solid (TSS), tot-N, tot-P
- Halogenoorganic compounds (AOX, TOX, TX, EOX, POX)
- Organic sulphur compounds (AOS, TS)
- Resin and chlororesin acids
- Saturated and unsaturated fatty acids
- Phenol and phenolic compounds (guaiacols, catechols, vanillin, veratrols)
- Tetrachlorophenol, Pentachlorophenol (PCP)
- Hexachlorocyclohexane (lindane)
- Aromatic and polyaromatic hydrocarbons
- Benzene, Hexachlorobenzene
- Phthalates
- Polychloro-Biphenyls (PCB)
- Carbohydrates
- Glyoxal
- Glycols
- Tin organic compounds

### Contact:

INSTITUTE OF BIOPOLYMERS AND CHEMICAL FIBRES  
ul. M. Skłodowskiej-Curie 19/27, 90-570 Łódź, Poland  
Małgorzata Michniewicz Ph. D.,  
tel. (+48 42) 638 03 31, e-mail: michniewicz@ibwch.lodz.pl